

1/8

SPECTRUM ANALYZER

FIG.1

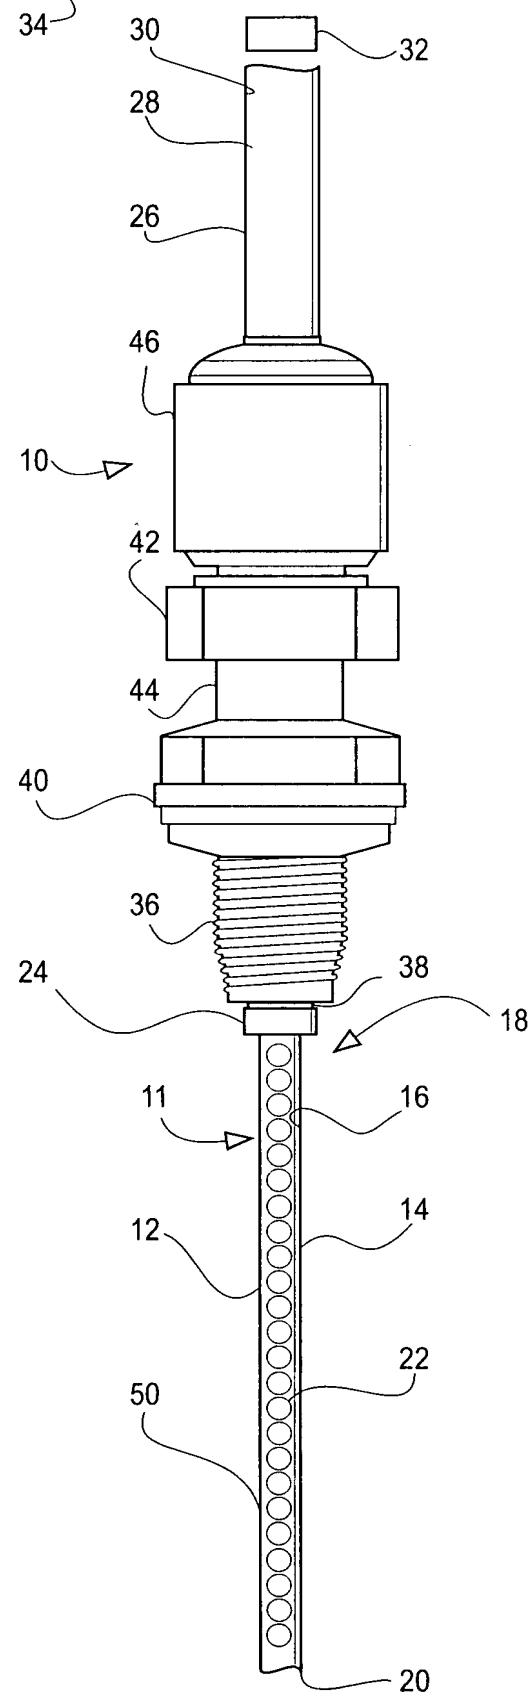


FIG. 2

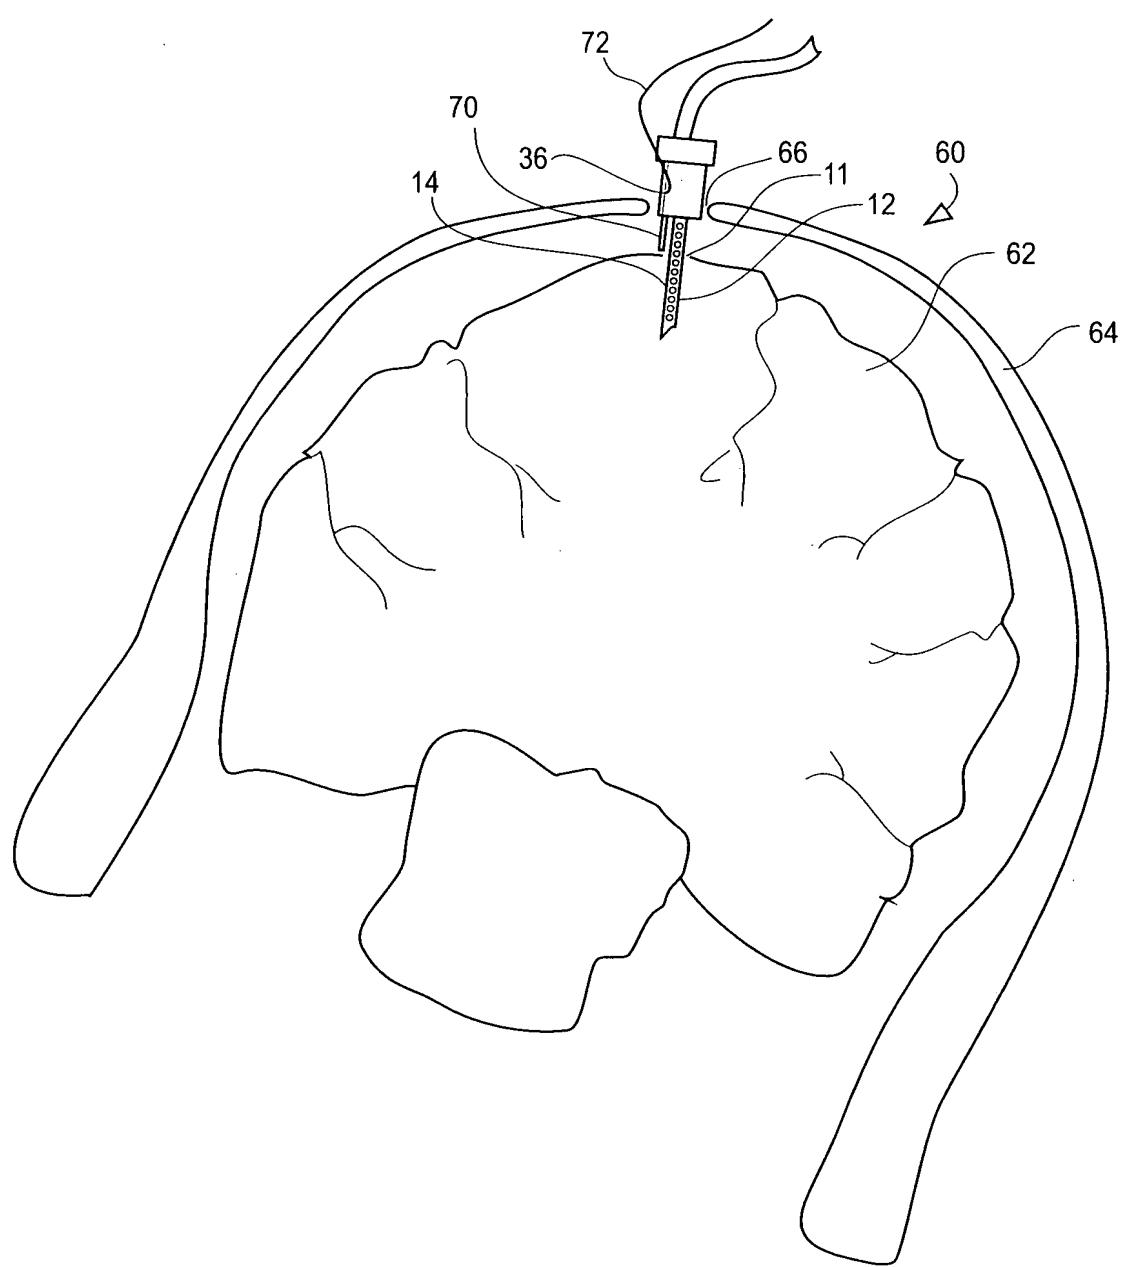


FIG. 3

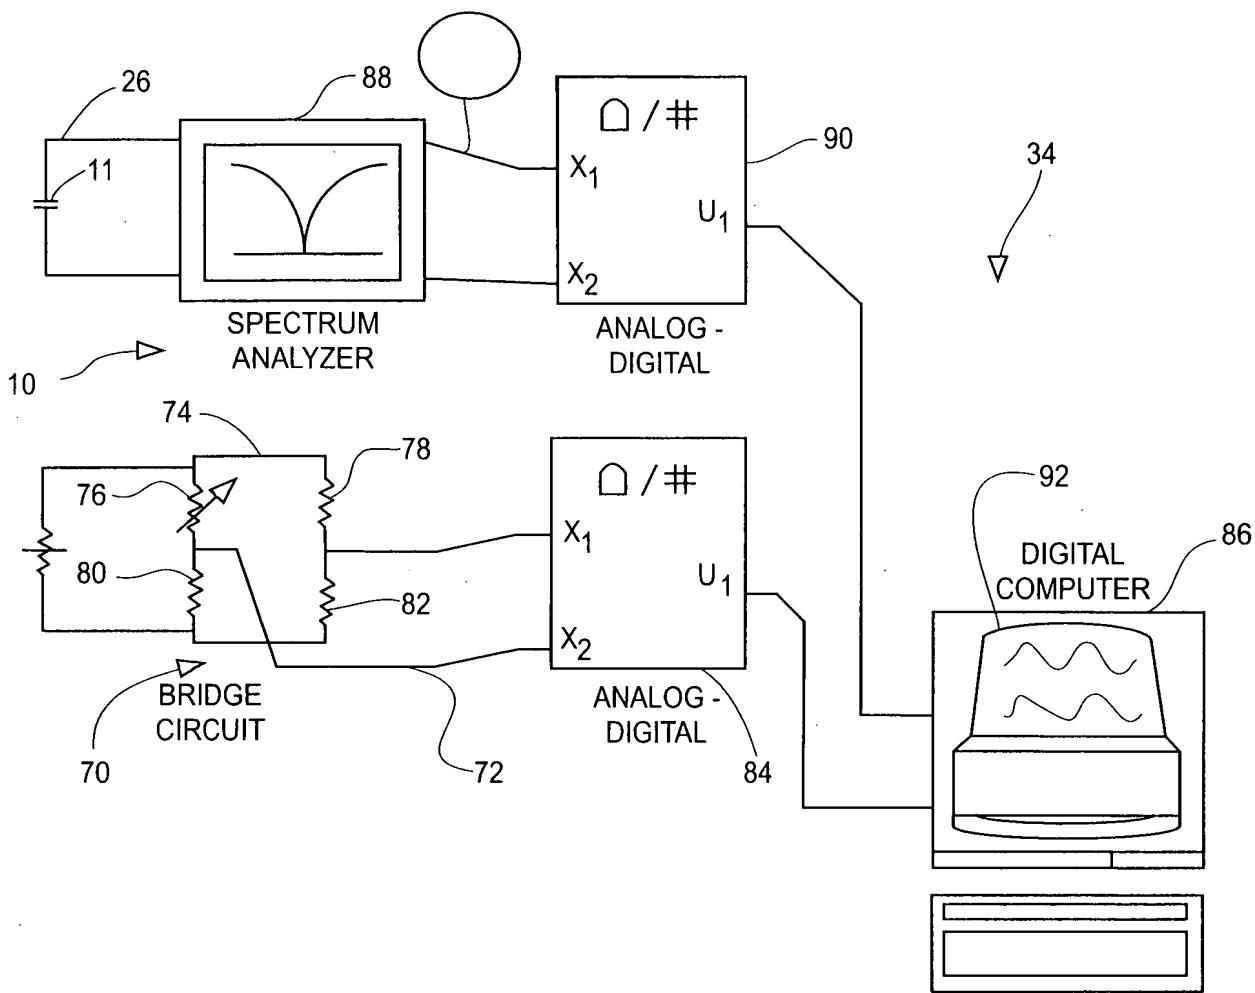


FIG. 4A

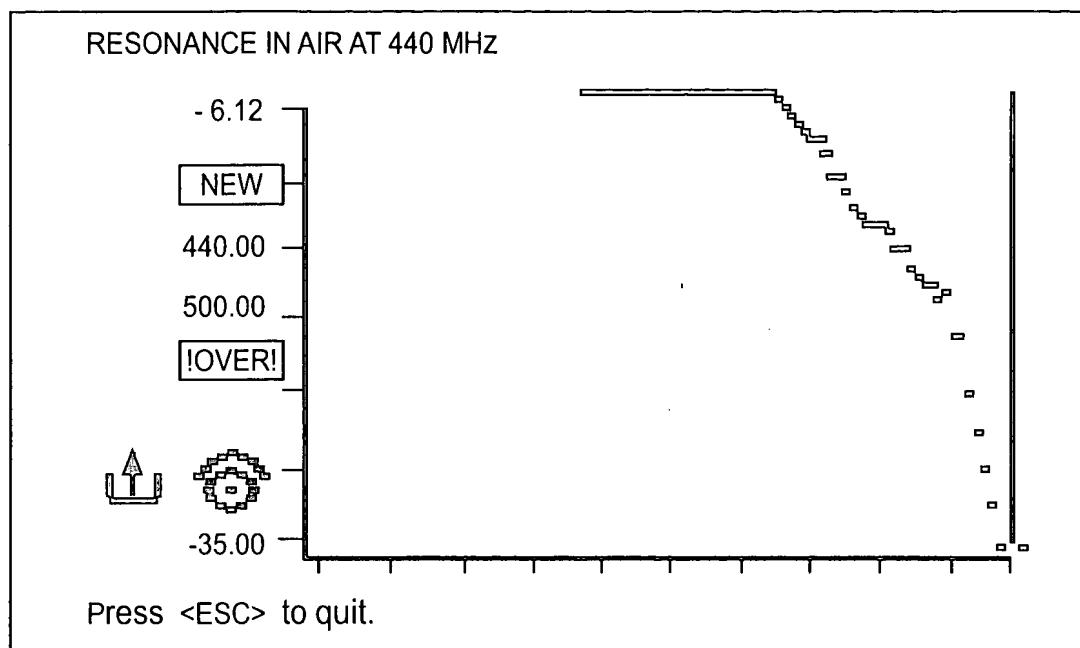


FIG. 4B

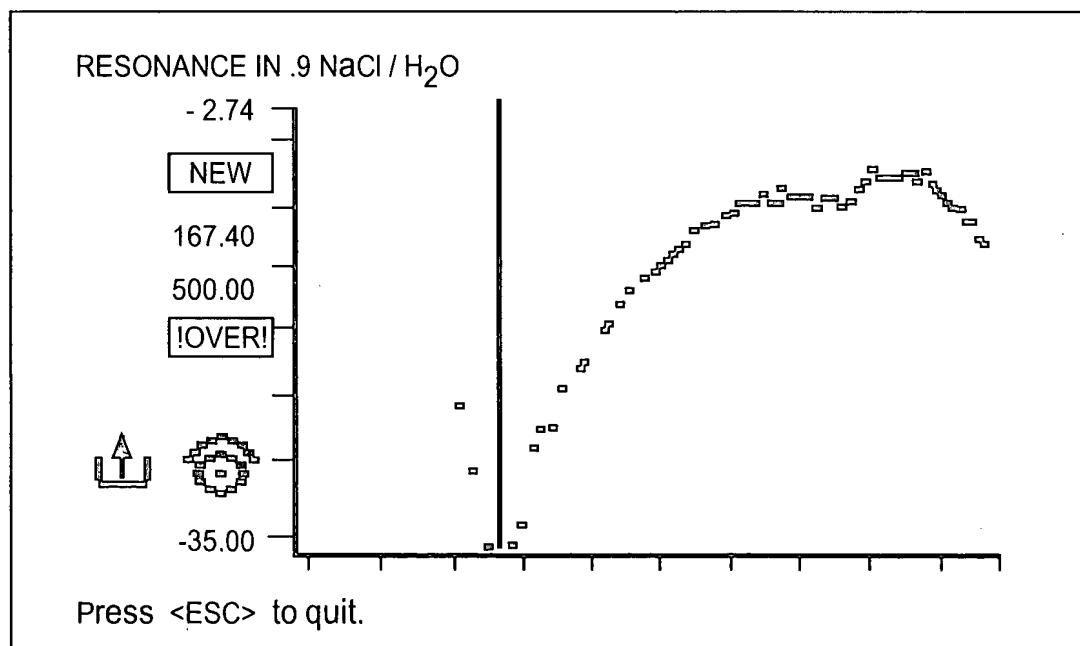


FIG. 4C

400 380 360 340 320 300 280 260 240 220 200

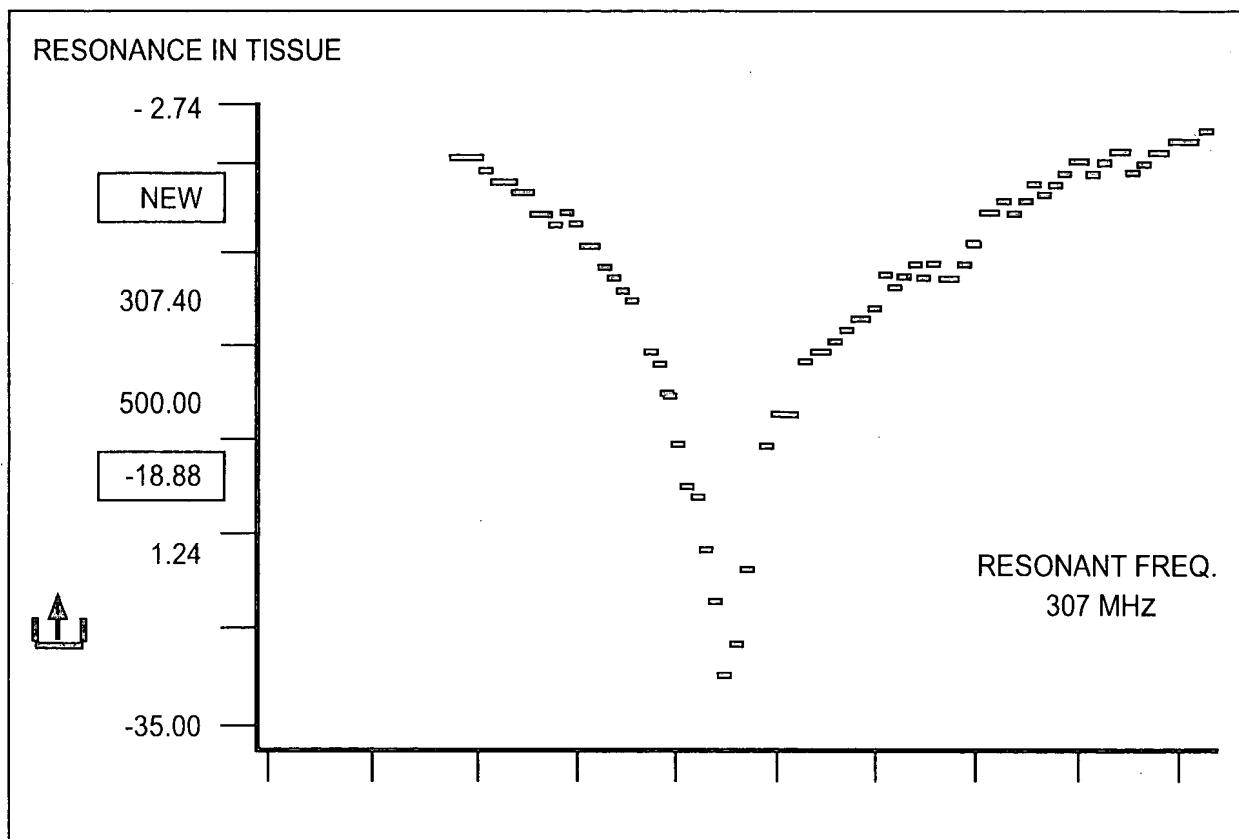


FIG. 4D


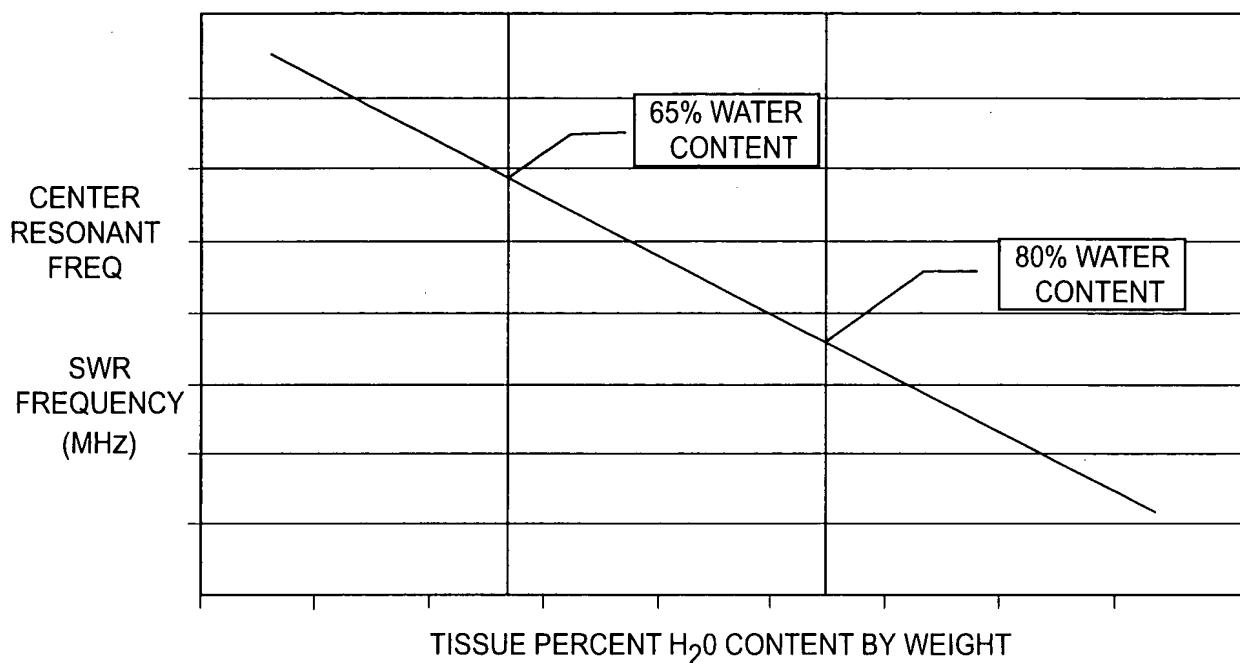
RELATIONSHIP OF H_2O CONTENT TO RESONANT FREQUENCY

FIG. 5

PULSATILE H_2O CONTENT PROBE OUTPUT
DUE TO CARDIAC PERFUSION OF THE BRAIN

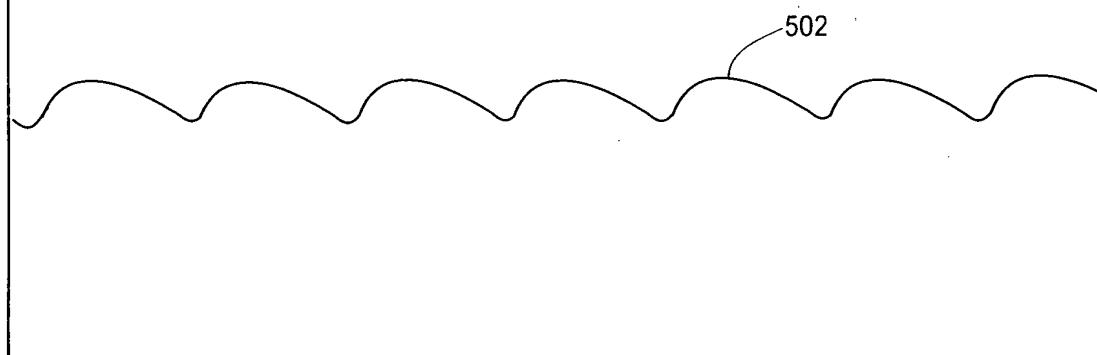

1000 900 800 700 600 500 400 300 200 100 0

FIG. 6

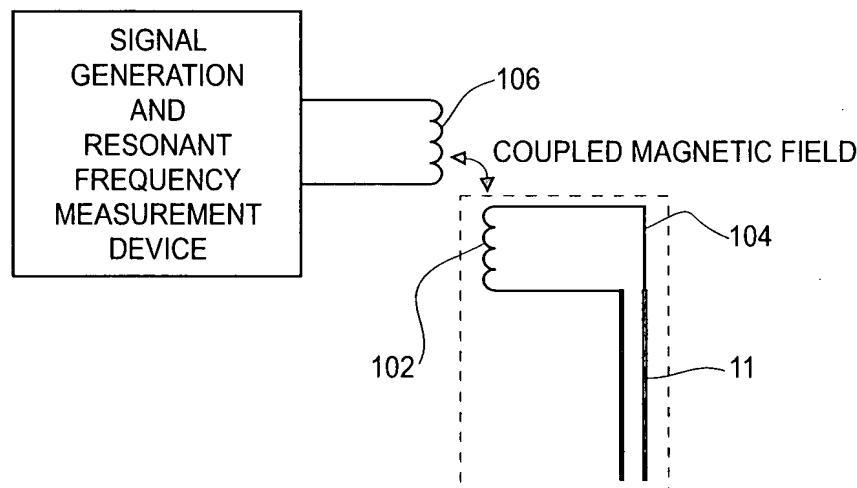


FIG. 7A

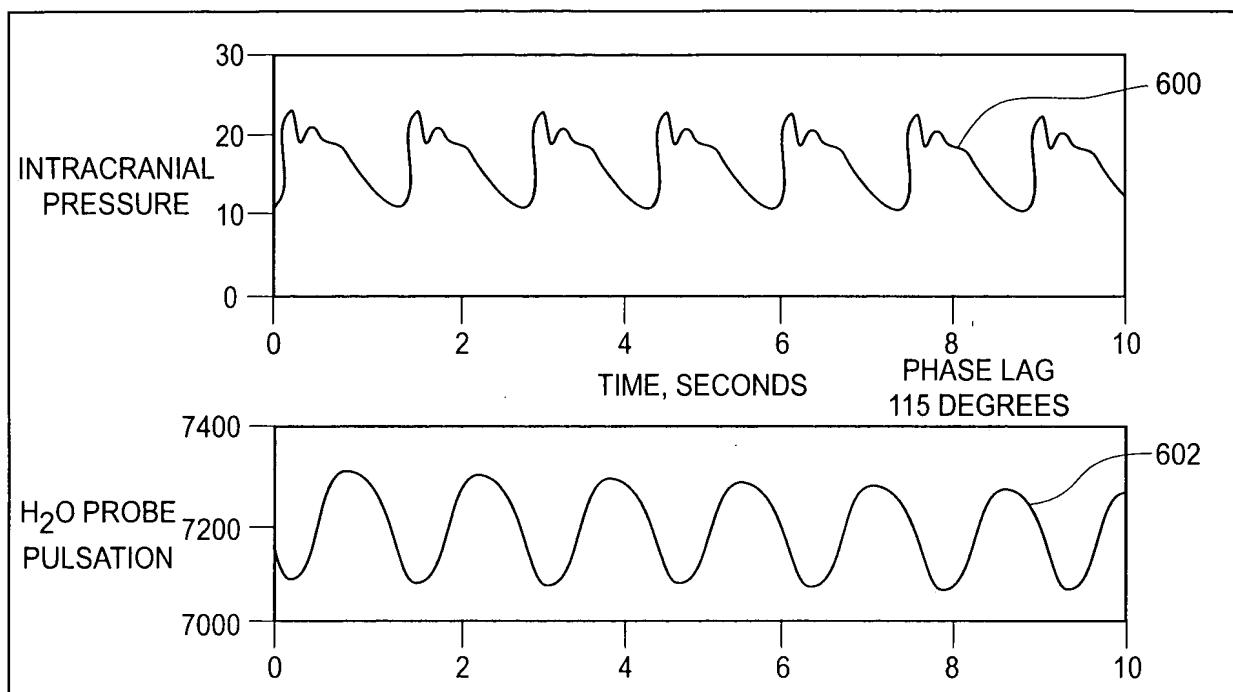


FIG. 7B

